
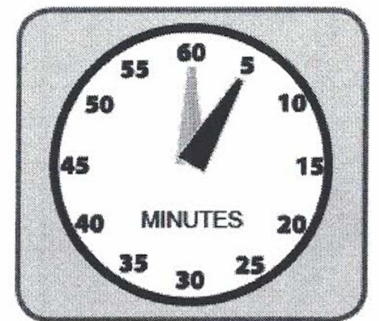
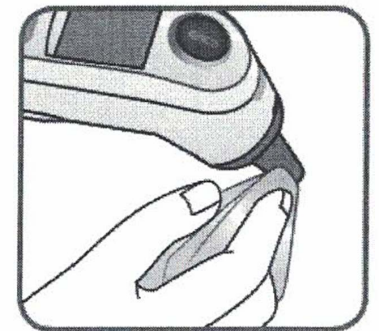







Cleaning the Probe Tip

- Gently wipe surface of probe lens window with cotton swab or cloth slightly moistened with **isopropyl or ethyl alcohol** only. Use gentle pressure.
- With probe facing down, wipe the probe with a damp cloth or cleaning wipe moistened with **isopropyl or ethyl alcohol**. Gently wipe with dry, clean cotton swab or cloth immediately.
- Allow at least **5 minutes** drying time before taking temperature. Make sure probe lens window is clean and dry prior to use.

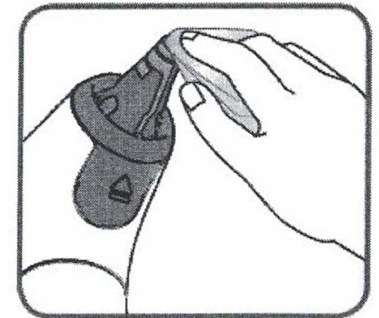

Cleaning the Body and Accessories

- For additional protection, place a new probe cover on the thermometer probe to protect this area when cleaning the body of the thermometer.
- Use a damp cloth or cleaning wipe with **cleaning solution from the Approved Cleaning Solutions Table**. To clean the body, ensure that the wipe is moist, not saturated. Wipe with display facing up.
- Clean accessories using same method. **Dry 5 min.**

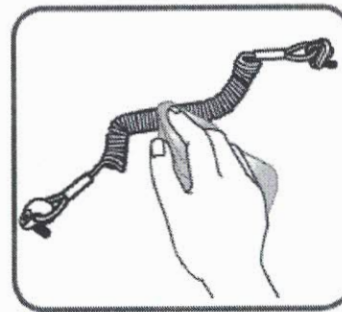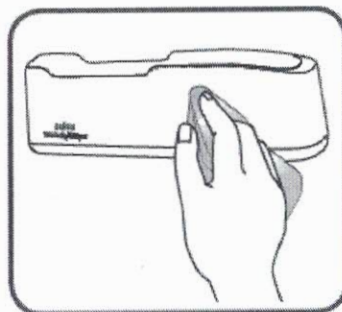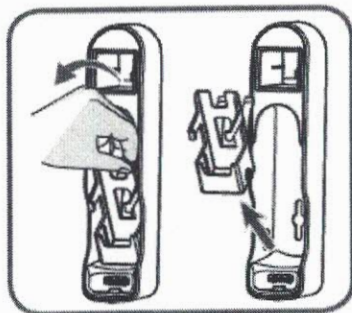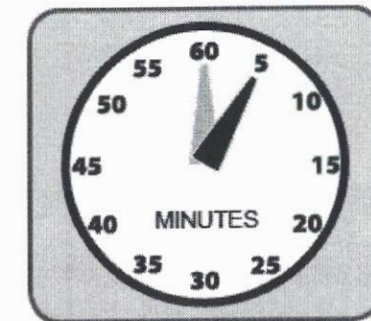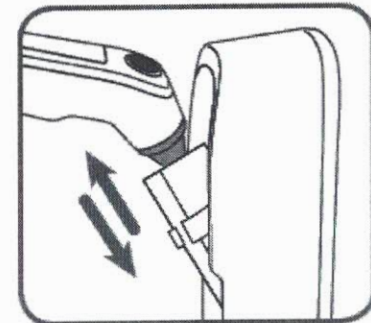

WelchAllyn®

Approved Cleaning Solutions

Approved cleaning solutions					
Family	Solution or Brand	Probe Lens Window	Probe	Thermometer Body & Cradle	Tether
Chlorine and Chlorine Compounds	10% Chlorine Bleach solution	No	No	Yes	Yes
Quaternary Ammonium Compounds	CaviWipes™	No	No	Yes	Yes
	Clinell® Universal Wipes				
	SaniCloth				
	Metrex				
Hydrogen Peroxide	Virox Oxivir	No	No	Yes	Yes
Alcohol	70% isopropyl or ethyl alcohol	Yes	Yes	Yes	Yes